


# Acrobat-i Off-Pump System

Positioning reference guide


# Acrobat-i Vacuum Stabilizer and Positioner System

## Blade mount


Left anterior descending artery

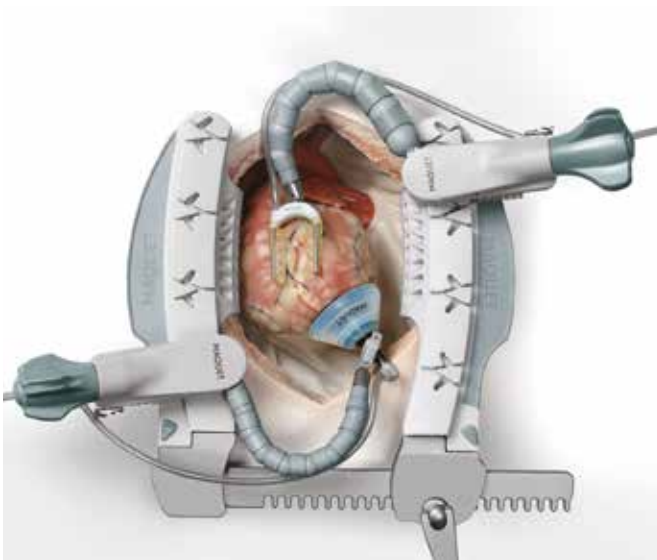


Right coronary artery

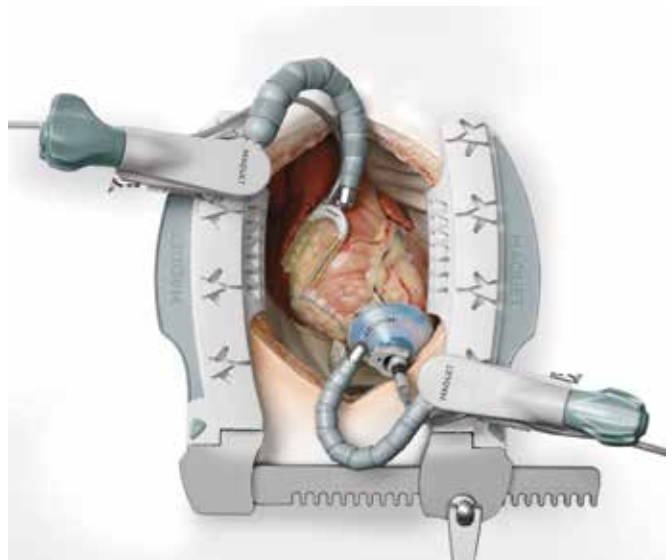

Posterior descending artery "toes-down"

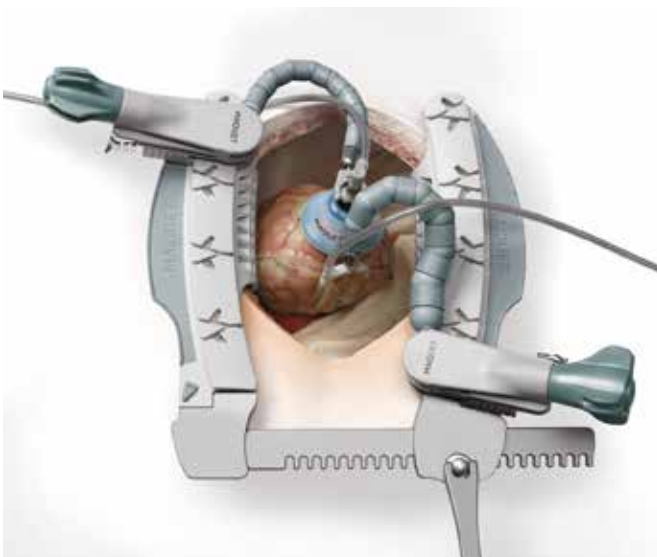


Posterior descending artery "toes-up"

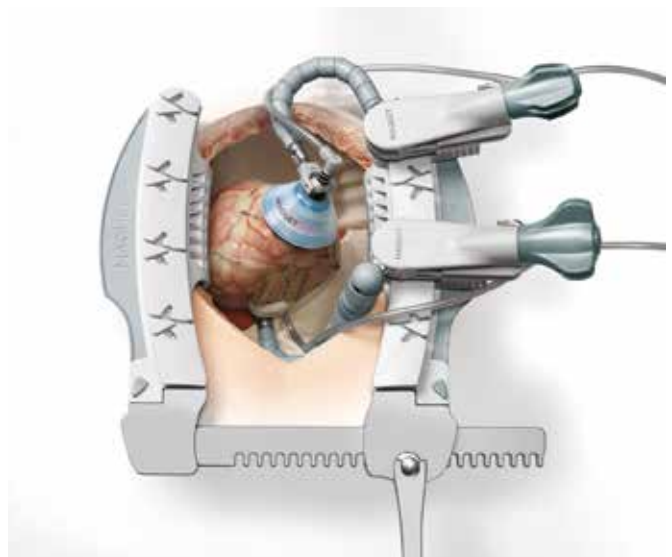


# Blade mount (continued)

Obtuse marginal branch "toes-up"

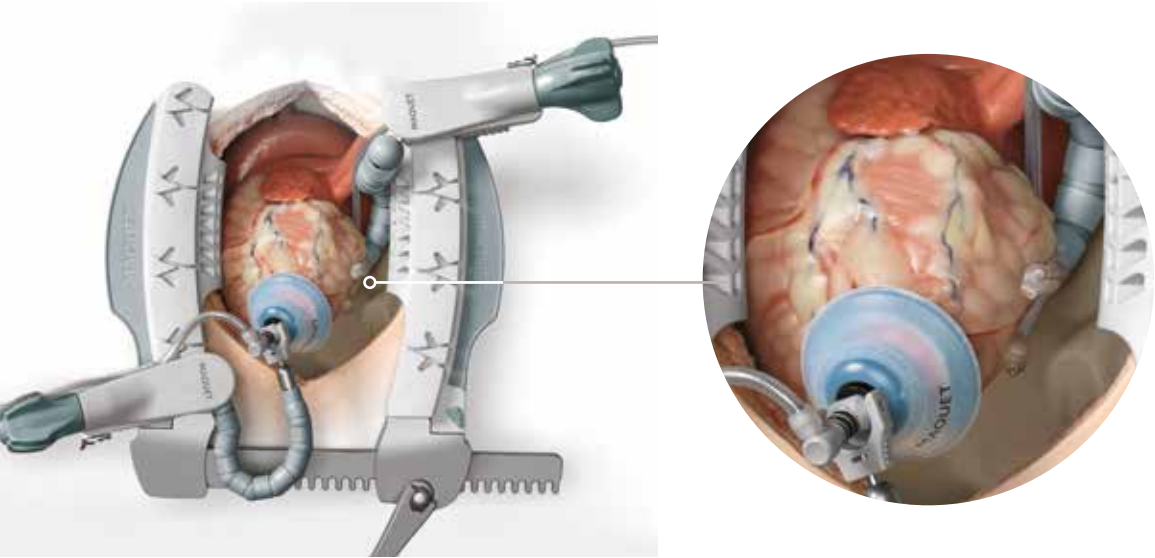


Obtuse marginal branch "toes-down"

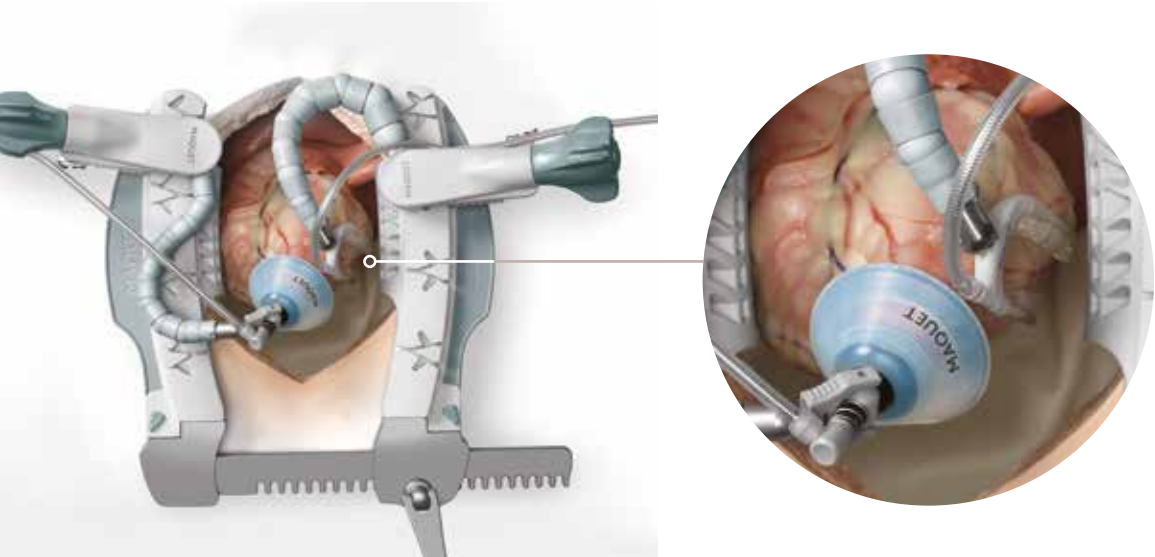


# Retractor mount

Obtuse marginal branch "toes-up" — retractor mount

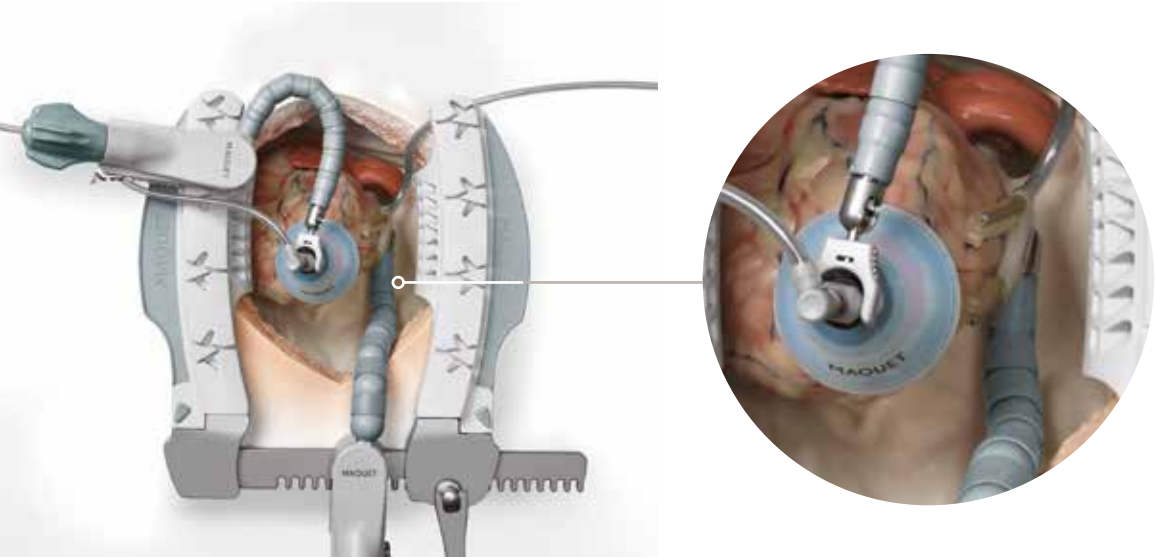


Obtuse marginal branch "toes-down" — retractor mount

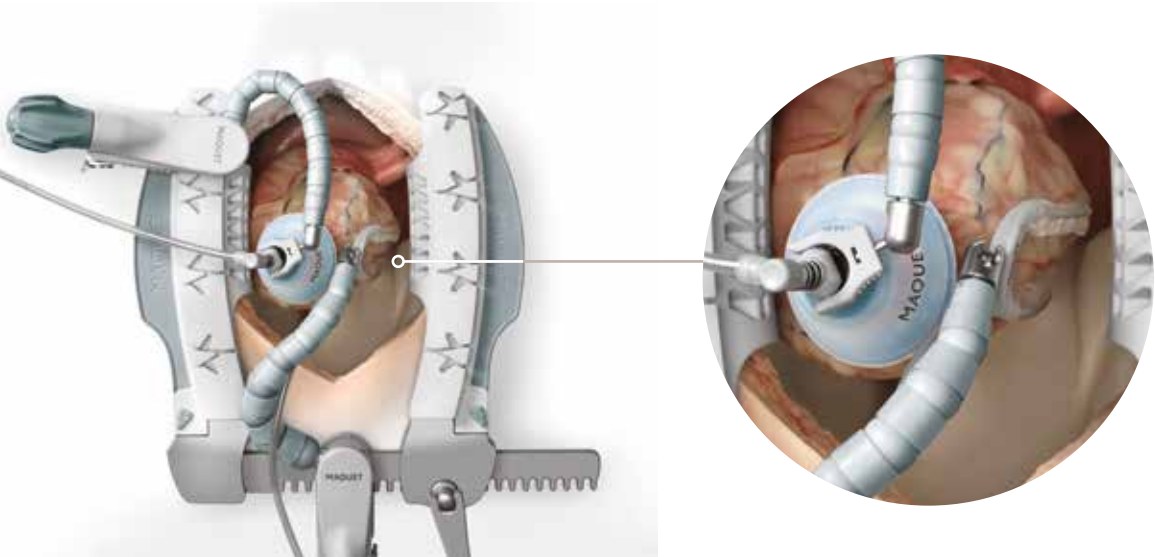


# Acrobat-i Off-Pump System

## Setup

### Acrobat-i Vacuum Stabilizer System

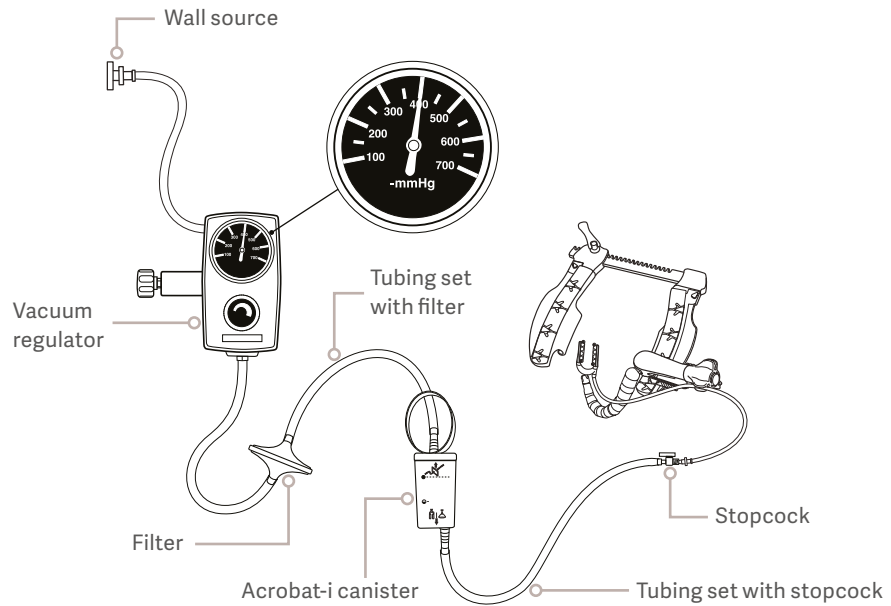

### Acrobat-i Vacuum Positioner System

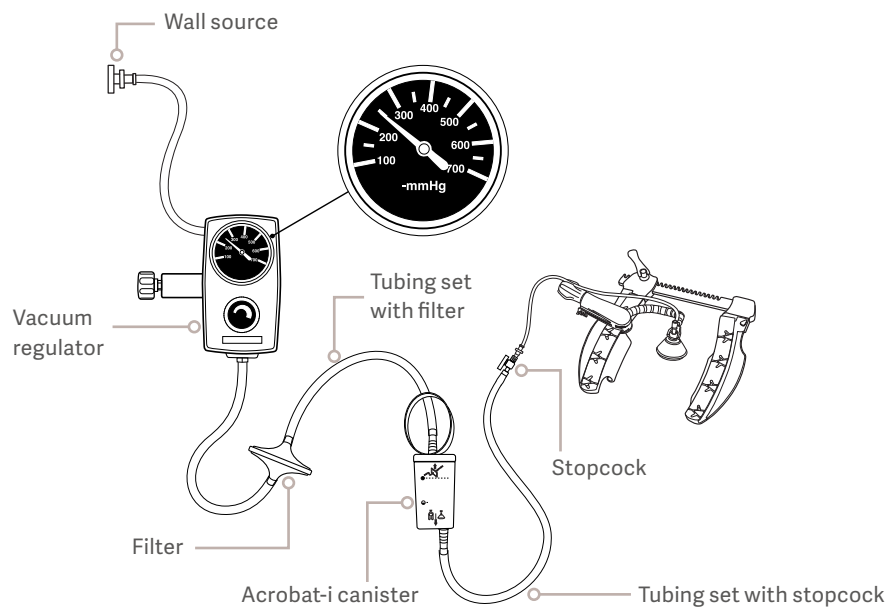



Getinge and **GETINGE** \* are registered trademarks of Getinge AB, its subsidiaries, or affiliates in the United States or other countries • Copyright 2020 Maquet Cardiovascular LLC • All rights reserved • ⚠ CAUTION: Federal (US) law restricts this device to sale by or on the order of a physician. Refer to Instructions for Use for current indications, warnings, contraindications, and precautions.

Getinge • 45 Barbour Pond Drive • Wayne, NJ 07470 • USA • 888 627 8383

[www.getinge.com](http://www.getinge.com)

MCV00020162 REVC