

Edi Catheter ENFit

- The new generation

Neurally Adjusted Ventilatory Assist (NAVA) and Neural Pressure Support (NPS) are modes of mechanical ventilation, where the ventilator is controlled directly by the patient's own neural respiratory drive.

The neural control of respiration originates in the respiratory center, where signals are transmitted through the phrenic nerve to create electrical activity of the diaphragm (Edi).

With NAVA and NPS, these signals are monitored using micro-electrodes in the Edi Catheter which are positioned in the esophagus at the level of the diaphragm.

A range of catheters in different French sizes and lengths, ensure optimized signal quality across all patient categories.



- New 6 Fr / 48 cm size for ELBW
- Usage time prolonged to 7 days

- Shelf-life prolonged to 3 years
- Revised neonatal weight range



- Updated labeling and instructions
- EU MDR 2017/745 certified



Patient group	Height (cm)	Bodyweight (kg)	Fr/cm	Material number (5pcs/pkg)
	<55	0.5-1.0	6/48	68 93 166
	<55	0.75-1.5	6/49	68 93 273
	<55	1.25-2.5	6/50	68 93 274
	<55	1.25-2.5	8/50	68 93 275
	45-85		8/100	68 93 276
	75-160		12/125	68 93 278
	>140		8/125	68 93 277
	>140		16/125	68 93 279

Edi catheter insertion and positioning


1. Connect the Edi module and cable.
2. Perform the Edi module function check.
3. Measure **NEX** (nose-ear and xiphoid) distance in cm.
4. Determine the insertion distance (use tape measure or on-screen calculator).
5. Dip the Edi catheter in water and insert.
6. Connect the Edi cable to catheter.
7. Verify the position in the catheter positioning window.
8. Check the position of the Edi catheter as a feeding tube according to hospital routines (e.g. X-ray, pH).
9. Secure it to the patient, and make a note of the insertion distance.
10. Verify the position regularly.

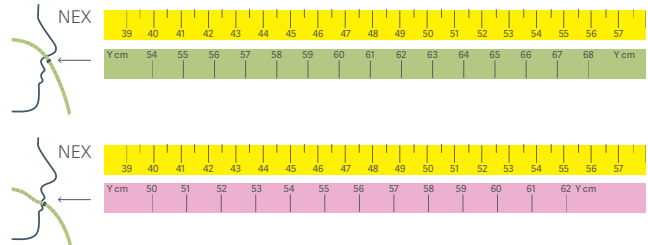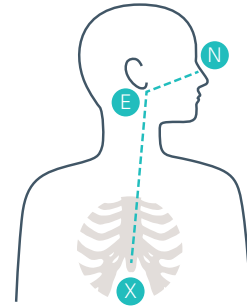

Positioning window


Note: The Edi catheter is positioned correctly if the second and third leads are highlighted in pink and the Edi signal is present.

An end- expiratory occlusion can also be made to check Edi signal versus patient's negative inspiratory pressure.

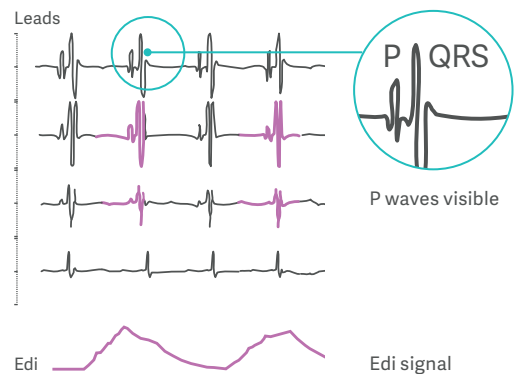

Edi Catheter ENFit

- Available for neonatal, pediatric, and adult patients
- Detect electrical activity of the diaphragm (Edi monitoring)
- Enable NAVA and NPS ventilation, both as invasive and non-invasive modes
- Also act as a normal nasogastric feeding tube
- Barium sulfate strip for x-ray identification
- Gamma sterilized
- Phthalate-free

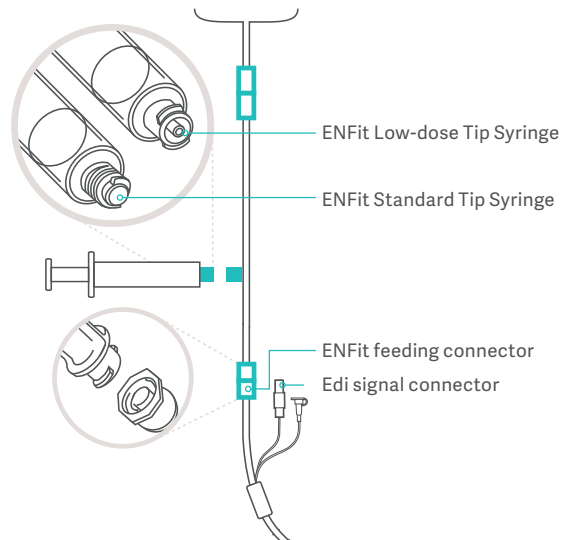

ISO 80369-3 – For further detailed information on the new enteral feeding system standard, visit www.stayconnected.org/

This information is aimed exclusively at healthcare professionals or other professional audiences and are for informational purposes only, is not exhaustive and therefore should not be relied upon as a replacement of the Instructions for Use, service manual or medical advice. Getinge shall bear no responsibility or liability for any action or omission of any party based upon this material, and reliance is solely at the user's risk.

Any therapy, solution or product mentioned might not be available or allowed in your country. Information may not be copied or used, in whole or in part, without written permission by Getinge.

Views, opinions, and assertions expressed are strictly those of the interviewed and do not necessarily reflect or represent the views of Getinge. The Edi Catheter ENFit may be pending regulatory approvals to be marketed in your country. Contact your Getinge representative for more information.

Manufacturer · Maquet Critical Care AB · Röntgenvägen 2 SE-171 54 Solna · Sweden · +46 (0)10 335 73 00

www.getinge.com

GETINGE