

Product Environmental Profile

Maquet Ezea Surgical Light

Overview

Getinge sustainability ambitions

At Getinge we take steps to empower our customers to reach their sustainability goals. One way to do this is by looking at how we can make our products and solutions as resource efficient as possible. We are committed to reduce our carbon footprint by setting ambitious targets to become net-zero by 2050 in line with the Science Based Targets initiative (SBTi).

All manufacturing sites work with environmental management systems in compliance with ISO 14001.

Read more about Getinge sustainability ambitions on our [website](#).

EcoDesign efforts

EcoDesign is standard practice at Getinge, focusing on using safer and fewer materials, incorporating circular solutions, and reducing media, energy, and water consumption.

The product was designed with a focus on minimizing both its mass and the number of components.

Product climate impact



The main cradle-to-grave results are representative for the EU market, please refer to page 5 for other regional scenarios.

Product description

Maquet Ezea Surgical Light offers user-friendly simplicity and robust reliability for a wide range of surgical applications or ambulatory surgery centers. It is designed to continuously align with evolving standards for risk management.

The profile has been achieved with:

- a dual Maquet Ezea 33DF 0810 configuration (2 cupolas + 2 spring arms + dual suspension)
- installation accessories (Flange 65, Tub 500 65)
- a power supply (EPS 20 B TR)
- 18 boxes of 5 HLX sterilizable handles.

Main assumptions of the Life Cycle Assessment study (LCI parameters)

The cupolas are adjusted to 100,000 Lux minimum and operate 10 hours per day, 300 days per year during 10 years. The electricity and water consumption used for the sterilization of the handles are part of this calculation.



Applicable directives and standards compliance for the product

1907/2006	REACH (Registration, Evaluation, Authorisation and Restriction of Chemicals)
60601-1-9 (2020)	Medical electrical equipment - Part 1-9
2011/65	ROHS Directives
2015/863	
2016/585	
2017/2102	
IEC 63000 (2022)	Technical documentation for the assessment of electrical and electronic products with respect to the restriction of hazardous substances.
US California proposition 65 Act (1986)	Health and Safety Code - HSC DIVISION 20. Miscellaneous Health and Safety Provisions Chapter 6.6. Safe Drinking Water and Toxic Enforcement Act of 1986.
SJ/T 11365 (2006)	ACPEIP - Administrative Measure on the Control of Pollution caused by Electronic Information Products Chinese RoHS (Restriction of Hazardous Substances).

Product

Total weight (net): 65.11 kg / 143.5 lbs



¹Electrical and Electronical Equipment - ²Polymethyl Methacrylate - ³Acrylonitrile Styrene Acrylate

Packaging

Total weight (gross): 21.84 kg / 48 lbs



Data input

The product was designed with a focus on minimizing both its mass and the number of components.

- Very low electricity consumption while in standby (for one light head): **<1W**
- Electrical consumption during operation (for one light head): **39.4W**
- CO₂ emissions compared to Maquet Lucea 100*: **-17%**
- Average electrical consumption compared to Maquet Lucea 100*: **-28%**

*Predecessor product

Recyclability




Recycled materials



The following materials are considered recyclable: Steel, Alu, Bronze, Brass, Copper (except cables), Cardboard, Paper, Thermoplastics (PMMA, PVC, ABS, PC, PS, PET, PE, PA, PP, POM). Thermosetting plastics, elastomers and other materials not listed are considered non recyclable. Recycled content evaluated in the study but requires documented trail in the value chain.


Supplier's location

The locations illustrated on this chart represent the origin of the suppliers utilized in the production of this product.

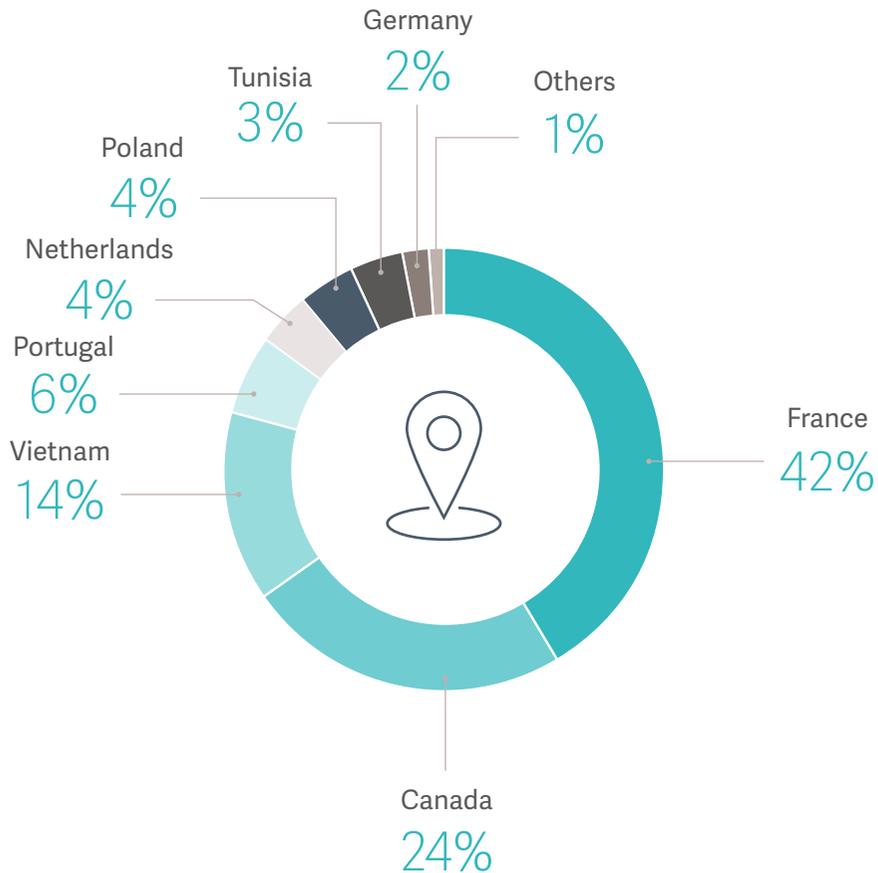

Environmental impacts

One point corresponds to the environmental impact of one person for one year. The result for this product is calculated over a period of 10 years.

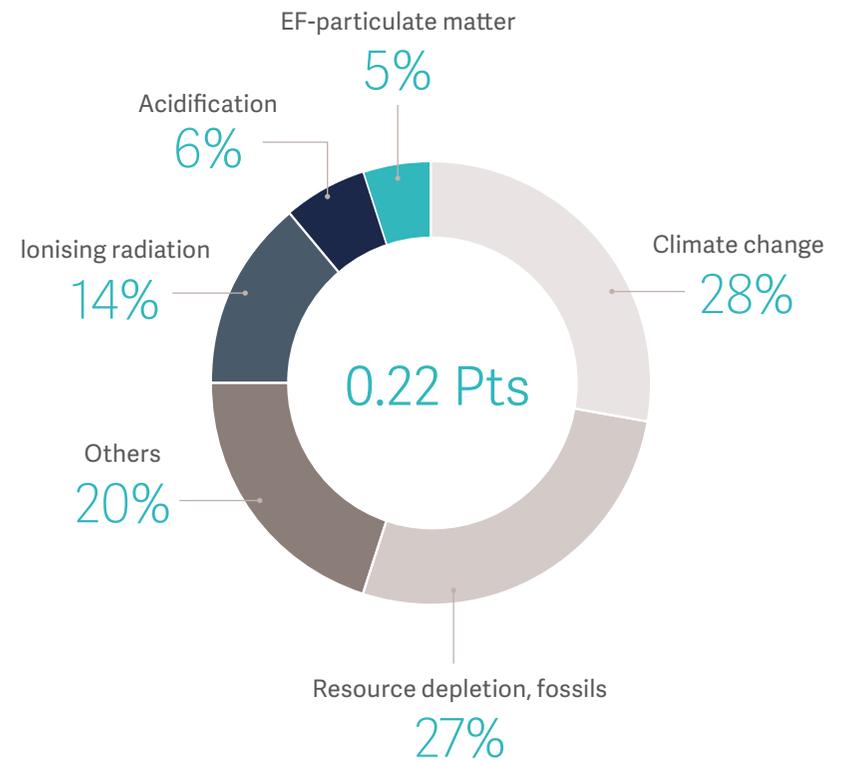

Product environmental impact with focus on climate impact

The main cradle-to-grave results are representative for the EU market and for other markets, please refer to regional scenarios. This as the results are sensitive to key parameters that are within the customer and end-user control and dependent on their geographical location such as choice of transportation mode and distances and waste handling of product and packaging.


Recommendations to reduce the climate impact

Recommendations to customers and end-users to further reduce the climate impact of their use of the product:

- Recycling of the product
- Switch-off your medical device when not in use
- Use low-carbon electricity
- Limit use of the maximum illumination

Global Warming Potential

t CO₂eq

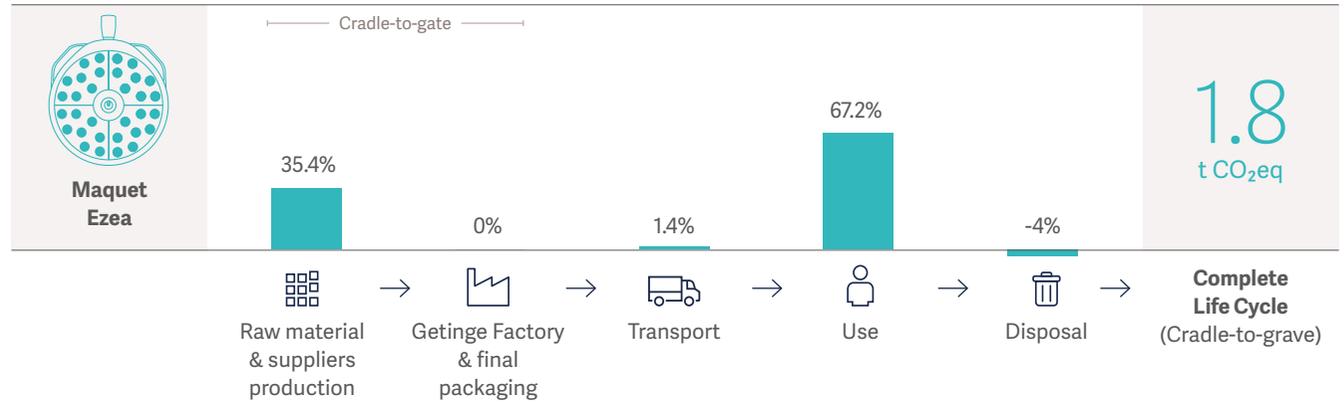

Regional scenarios t CO₂eq

Europe	35.4%	0%	1.4%	67.2%	-4%	1.8 t CO₂eq
North America*	28.8%	0%	1.4%	73%	-3.2%	2.2 t CO₂eq
South America**	54.7%	0%	2.6%	48.8%	-6.1%	1.2 t CO₂eq
APAC***	21.9%	0%	1.1%	79.5%	-2.5%	2.9 t CO₂eq
Middle East	21.3%	0%	1%	80.1%	-2.4%	3.5 t CO₂eq
Japan	27.3%	0%	1.3%	74.4%	-3%	2.3 t CO₂eq
Low carbon energy	97.3%	0%	4.7%	8.9%	-10.9%	0.7 t CO₂eq

*Based on US data


**Based on Brazilian data

***Based on Chinese data

Complete life cycle per region

For indication, the emission of 2 t CO₂eq is equivalent to:

- a car travel of 9,191 km (thermic car)
- a train travel of 847,458 km
- 13 laptops

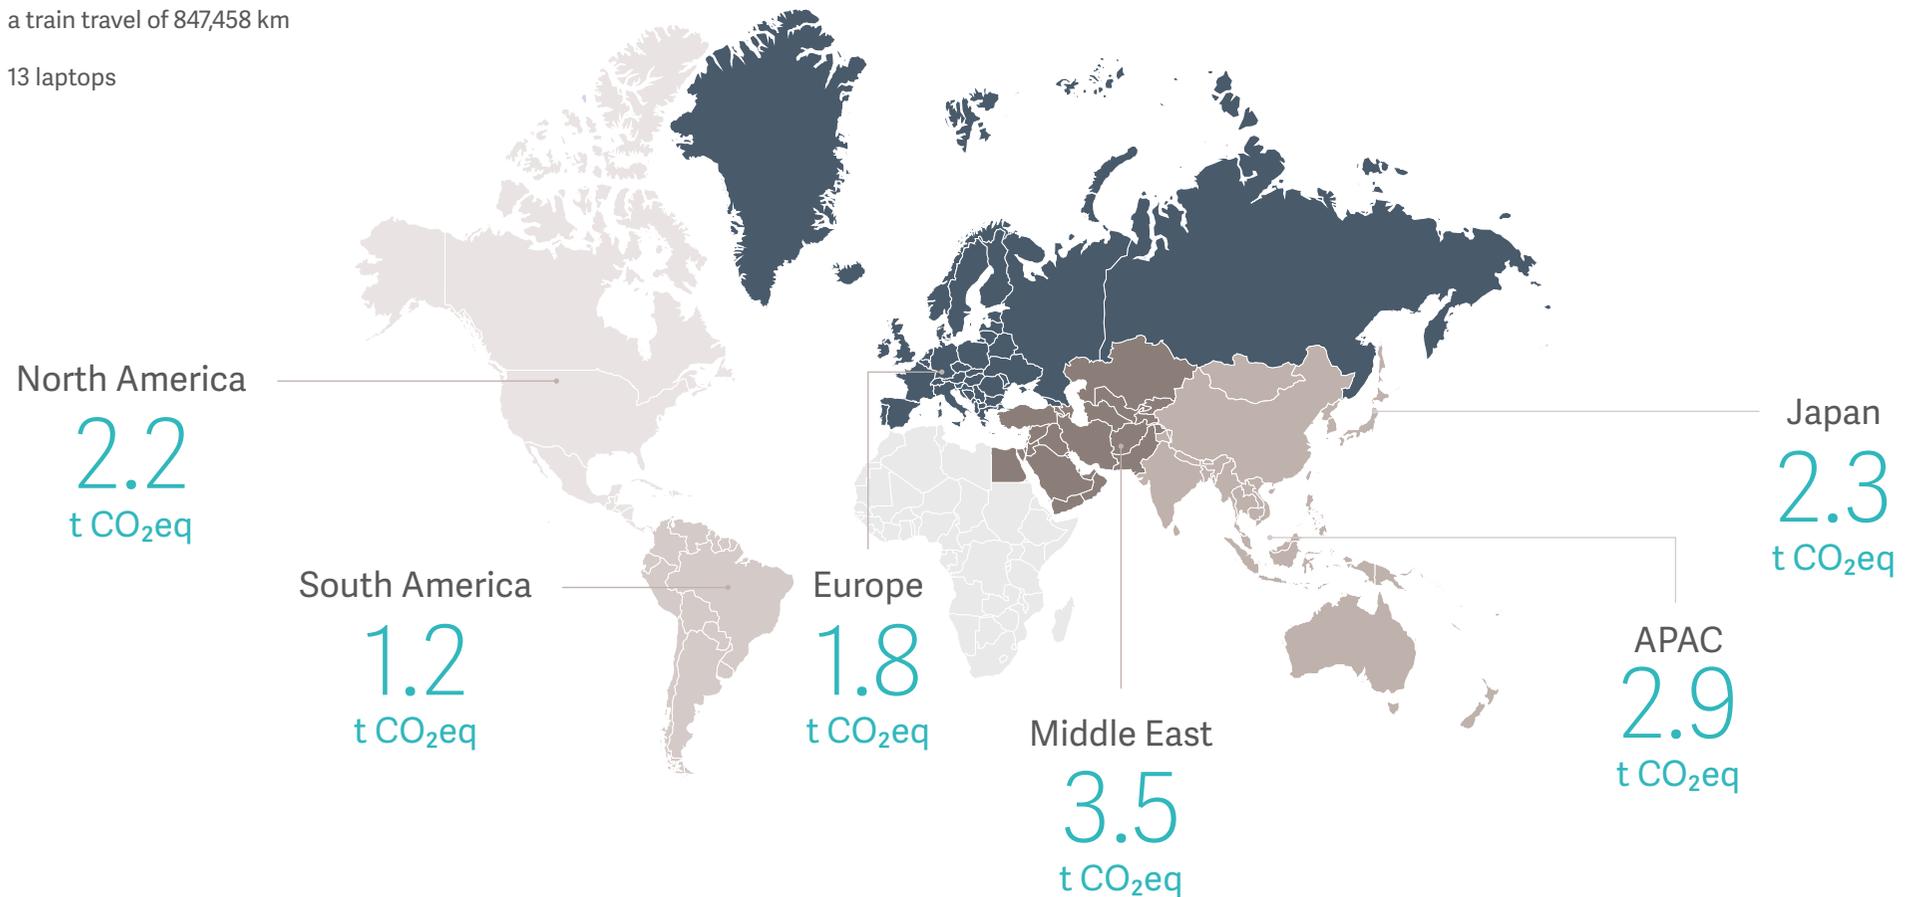

The LCA and EcoDesign methods

Product Environmental Profile (PEP) communicates the results of a Life Cycle Assessment (LCA). This is a methodology for assessing environmental impacts associated with all the stages of the life cycle of a product, process, or service. I.e. for a product environmental impacts are assessed for the raw material extraction (cradle) followed by the whole value-chain further processing, through the product's manufacturing (gate), distribution and use, to the recycling or final disposal of the materials it is composed of.

The EIME (Environmental Impact and Management Explorer) software, version 6.1.1, and its database (version CODDE-2023-02) were used for the Life Cycle Assessment (LCA). Indicators from the PEP Ecopassport PCR3 – 2015 were applied. All LCA studies include holistic analysis of all relevant environmental impacts used for EcoDesign input. Further details can be available upon request, contact responsible PLM/R&D team.



This information is intended for an international audience outside the US.

This information is aimed exclusively at healthcare professionals or other professional audiences and are for informational purposes only, is not exhaustive and therefore should not be relied upon as a replacement of the Instructions for Use, service manual or medical advice. Getinge shall bear no responsibility or liability for any action or omission of any party based upon this material, and reliance is solely at the user's risk.

Any therapy, solution or product mentioned might not be available or allowed in your country. Information may not be copied or used, in whole or in part, without written permission by Getinge.

Manufacturer: Maquet S.A.S · Parc de Limère · Avenue de la Pomme de Pin · CS 10008 Ardon · 45074 Orléans, cedex 2 · France

© 2025 Getinge | Getinge and **GETINGE**  are trademarks or registered trademarks of Getinge AB, its subsidiaries or affiliates.
DMS-0009075 v3 | All rights reserved.